

Chapter 36

Brain–Machine Interface Using Brain Surface Electrodes: Real–Time Robotic Control and a Fully Implantable Wireless System

Masayuki Hirata

Osaka University Medical School, Japan

Hiroshi Yokoi

The University of Tokyo, Japan

Takufumi Yanagisawa

Osaka University Medical School, Japan

Tetsu Goto

Osaka University Medical School, Japan

Kojiro Matsushita

Osaka University Medical School, Japan

Morris Shayne

Osaka University Medical School, Japan

Hisato Sugata

Osaka University Medical School, Japan

Youichi Saitoh

Osaka University Medical School, Japan

Yukiyasu Kamitani

*ATR Computational Neuroscience
Laboratories, Japan*

Haruhiko Kishima

Osaka University Medical School, Japan

Takafumi Suzuki

*National Institute of Information and
Communications Technology, Japan*

Mitsuo Kawato

*ATR Computational Neuroscience
Laboratories, Japan*

Toshiki Yoshimine

Osaka University Medical School, Japan

ABSTRACT

The brain-machine interface (BMI) enables us to control machines and to communicate with others, not with the use of input devices, but through the direct use of brain signals. This chapter describes the integrative approach the authors used to develop a BMI system with brain surface electrodes for real-time robotic arm control in severely disabled people, such as amyotrophic lateral sclerosis patients. This integrative BMI approach includes effective brain signal recording, accurate neural decoding, robust robotic control, a wireless and fully implantable device, and a noninvasive evaluation of surgical indications.

DOI: 10.4018/978-1-4666-2196-1.ch036
cal indications.

INTRODUCTION

The brain-machine interface (BMI) is a man-machine interface that enables us to control machines and to communicate with others not with the use of input devices, but through the direct use of brain signals alone (Figure 1). Several diseases and conditions can lead to the loss of muscular control without a disruption in patients' brain function, including amyotrophic lateral sclerosis (ALS), brainstem stroke, spinal cord injury, and muscular dystrophy, among others. BMI technology offers these patients greater independence and a higher quality of life by enabling the control of external devices to communicate with others and the ability to manipulate their environment at will (Wolpaw, Birbaumer, McFarland, Pfurtscheller, & Vaughan, 2002).

There are two types of BMI: invasive BMI and noninvasive BMI. Invasive BMI requires

surgical procedures and measures the brain signals from intracranial electrodes (needle electrodes or brain surface electrodes), whereas noninvasive BMI measures brain signals noninvasively from outside of the body using scalp electrodes, and so forth. To achieve a higher performance and a higher level of usefulness, we employed invasive BMI techniques, which involve the implantation of devices. For use in a practical situation, invasive BMI requires an organic integration of the following medical and engineering technologies:

1. Neural recording with high spatiotemporal resolution.
2. High-speed data transfer and processing.
3. Optimal extraction of appropriate neurophysiological features.
4. Accurate neural decoding.
5. Robust control of external devices such as robotic arms and electric wheelchairs.
6. Downsizing, integration, and implantation of electronic devices, and the use of wireless technology.
7. Noninvasive pre-surgical evaluations for appropriate surgical indications.
8. On-target survey and analysis of patient needs.
9. Addressing of neuroethical issues.


In this chapter, we describe the development of our invasive BMI system using brain surface electrodes.

NEURAL DECODING AND REAL-TIME ROBOTIC CONTROL USING ELECTROCORTICOGRAMS

Clinical Studies Using Electroencephalograms Recorded from Brain Surface Electrodes

In the process of providing neurosurgical treatments for specific groups of patients, we some-

Figure 1. A conceptual diagram of the brain machine interface

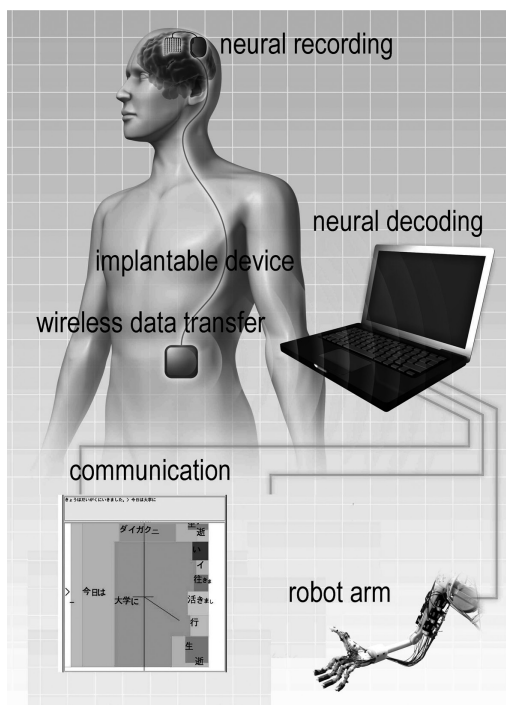

11 more pages are available in the full version of this document, which may be purchased using the "Add to Cart" button on the publisher's webpage:

www.igi-global.com/chapter/brain-machine-interface-using-brain/70877

Related Content

Relationship Between Speed of Performing Leg Extension With 30 RM Load and the Selected EMG Variables of Selected Quadricep Muscles

Dhananjoy Shaw, Deepak Singh, Umesh Kumar Ahlawat, Manvinder Kaur and Dinesh Bhatia (2021).

International Journal of Biomedical and Clinical Engineering (pp. 61-76).

www.irma-international.org/article/relationship-between-speed-of-performing-leg-extension-with-30-rm-load-and-the-selected-emg-variables-of-selected-quadricep-muscles/272063

Use of Telemedicine Systems and Devices for Patient Monitoring

Dionisia Damigou (2009). *Medical Informatics: Concepts, Methodologies, Tools, and Applications* (pp. 733-739).

www.irma-international.org/chapter/use-telemedicine-systems-devices-patient/26253

Handling Large Medical Data Sets for Disease Detection

Rahul Kala, Anupam Shukla and Ritu Tiwari (2011). *Biomedical Engineering and Information Systems: Technologies, Tools and Applications* (pp. 162-176).

www.irma-international.org/chapter/handling-large-medical-data-sets/43298

Telederm: A Web-Based Decision Support System for Medical Practitioners

Geoff West, Mihai Lazarescu and Monica Ou (2010). *Biomedical Knowledge Management: Infrastructures and Processes for E-Health Systems* (pp. 154-176).

www.irma-international.org/chapter/telederm-web-based-decision-support/42605

Low Noise EEG Amplifier Board for Low Cost Wearable BCI Devices

Ravimand Suma K. V. (2016). *International Journal of Biomedical and Clinical Engineering* (pp. 17-28).

www.irma-international.org/article/low-noise-eeeg-amplifier-board-for-low-cost-wearable-bci-devices/170459